



SCOPE OF ACCREDITATION TO ISO/IEC 17025:2005

BRIGHTON-BEST INTERNATIONAL INC.  
Laboratory Testing Division  
2100 Center Square Rd  
Logan Township, NJ 08085  
Chuck Halpin Phone: 856 241 9494

MECHANICAL

Valid To: July 31, 2019

Certificate Number: 0616.01

In recognition of the successful completion of the A2LA evaluation process, accreditation is granted to this laboratory to perform the following fastener tests:

**Test**

**Test Methods**

Hardness (Rockwell C)

ASTM E18, F606/F606M; ISO 898-1

Dimensional Testing<sup>1</sup>


Parameter	Range	CMC <sup>2</sup> (±)	Technique / Method
Threads <sup>3</sup>			
External	4-40 to 1.000 in #8 to 1 in	0.0005 in N/A	Tri-roll gage/ IFI Hbk 7 <sup>th</sup> Ed. ASME B1.3 screw thread gaging systems, go/no-go ring gages
Internal	0.25 to 1.5 in	N/A	ASME B1.3 System 21 Thread plug go/no-go
Socket Recess <sup>3</sup>	Up to 0.5000 in	0.0009 in	Recess checker gage (indicator)/ IFI Hbk 7 <sup>th</sup> Ed.
Radii <sup>3</sup>	Up to 6.000 in	0.001 in	Optical comparator/ IFI Hbk 7 <sup>th</sup> Ed.
Angle <sup>3</sup>	Up to 360°	0.08°	Optical comparator/ IFI Hbk 7 <sup>th</sup> Ed.

Parameter	Range	CMC <sup>2</sup> (±)	Technique / Method
Linear <sup>3</sup>	Up to 1.0000 in	0.0005 in	Micrometer/ IFI Hbk 7 <sup>th</sup> Ed
	Up to 6.0000 in	0.0007 in	Caliper/ IFI Hbk 7 <sup>th</sup> Ed.
	Up to 6.0000 in	0.0007 in	Optical comparator/ IFI Hbk 7 <sup>th</sup> Ed.
Protrusion Gaging <sup>3</sup>	Up to 1.0000 in	0.0005 in	Indicator/ IFI Hbk 7 <sup>th</sup> ED
Camber/Straightness <sup>3</sup>	Up to 1.000 in	0.001 in	ASME B18.2.9

<sup>1</sup> This laboratory does not offer commercial dimensional testing services.

<sup>2</sup> Calibration and Measurement Capability (CMC) is the smallest uncertainty of measurement that a laboratory can achieve within its scope of accreditation when performing more or less routine measurements of nearly ideal measurement standards or nearly ideal measuring equipment. CMCs represent expanded uncertainties expressed at approximately the 95 % level of confidence, usually using a coverage factor of  $k = 2$ . The actual measurement uncertainty of a specific measurement performed by the laboratory may be greater than the CMC due to the behavior of the customer's device and to influences from the circumstances of the specific measurement.

<sup>3</sup> This test is not equivalent to that of a calibration.

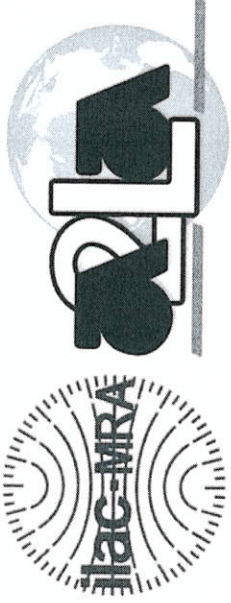

# Accredited Laboratory

A2LA has accredited

## BRIGHTON-BEST INTERNATIONAL INC.

Logan Township, NJ

for technical competence in the field of

### Mechanical Testing

This laboratory is accredited in accordance with the recognized International Standard ISO/IEC 17025:2005 General requirements for the competence of testing and calibration laboratories. This accreditation demonstrates technical competence for a defined scope and the operation of a laboratory quality management system (refer to joint ISO-IAC-IAF Communiqué dated 8 January 2009).



Presented this 29<sup>th</sup> day of August 2017.

A handwritten signature in black ink, appearing to read 'L. ...', positioned above a horizontal line.

President and CEO  
For the Accreditation Council  
Certificate Number 0616.01  
Valid to July 31, 2019